

gloveon Paloma

Nitrile Exam Gloves Powder Free, Standard Cuff

Like the purity of a white Dove, **Paloma**, our white nitrile gloves offers the elegance of touch and feel with strength and dexterity needed for the delicate procedure and jobs.



| GloveOn Paloma | | |
|------------------------------------|-------------------------|---------------------|
| Length (mm) | ≥ 230 | |
| Thickness Measurements (mm) | | |
| Palm (centre of Palm) | 0.07 ± 0.02 | |
| Finger (13mm ± 3mm from tip) | 0.09 ± 0.02 | |
| Physical Properties | Before Ageing | After Ageing |
| Tensile Strength (MPa) | ≥ 18 | ≥ 16 |
| Elongation (%) | ≥ 500 | ≥ 400 |
| Inspection Levels & AQL | Inspection Level | AQL |
| Watertightness | G1 | 1.50 |
| Physical Dimensions | S2 | 4.00 |
| Tensile Strength | S2 | 4.00 |
| Visual Inspection (Major) | S4 | 2.50 |
| Visual Inspection (Minor) | S4 | 4.00 |
| Particulate Residue | N = 5 | ≤ 2mg/glove |

| Chemotherapy Drugs and Concentration (Tested for Resistance to Permeation by Chemotherapy Drugs as per ASTM D6978-05 Test Report PN 116668) | Minimum Breakthrough Detection Time (minutes) |
|---|--|
| Carmustine (BCNU), 3.3mg/ml (3,300 ppm) | 15.1 minutes |
| Cisplatin, 1.0mg/ml (1,000 ppm) | >240 minutes |
| Cyclophosphamide (Cytoxan), 20.0mg/ml (20,000 ppm) | >240 minutes |
| Dacarbazine (DTIC), 10.0mg/ml (10,000 ppm) | >240 minutes |
| Doxorubicin Hydrochloride, 2.0mg/ml (2,000 ppm) | >240 minutes |
| Etoposide (Toposar), 20.00mg/ml (20,000 ppm) | >240 minutes |
| Fluorouracil, 50.0mg/ml (50,000 ppm) | >240 minutes |
| Methotrexate, 25.0mg/ml (25,000 ppm) | >240 minutes |
| Mitomycin C, 0.5mg/ml (500 ppm) | >240 minutes |
| Paclitaxel (Taxol), 6.0mg/ml (6,000 ppm) | >240 minutes |
| Thiotepa, 10.0mg/ml (10,000 ppm) | 15.4 minutes |
| Vincristine Sulfate, 1.0mg/ml (1,000 ppm) | >240 minutes |

REORDER CODE

| | |
|---------|---------|
| NTR51XS | X-SMALL |
| NTR51SS | SMALL |
| NTR51MM | MEDIUM |
| NTR51LL | LARGE |
| NTR51XL | X-LARGE |

FEATURES

- Fingertip textured
- Powder free
- Not made with natural rubber latex
- Chemo drugs tested
- Lab chemical tested
- Ambidextrous
- Standard cuff
- White colour

PACKAGING

200 gloves per box for XS to L
180 gloves per box for XL
10 boxes per carton

REGULATORY COMPLIANCE

TGA - ARTG 164563, FDA 510(k),
MDD 93/42/EEC, REACH,
ROHS Directive 2002/95/EC, EC 10/2011,
REGULATION (EC) No 1935/2004,
PPE 89/686/EEC

STANDARDS

ASTM D6319, EN 455 part 1, 2, 3 & 4,
EN 1186, EN 13130, CEN/TS 14234,
EN 420, EN 374 part 1, 2 & 3

MANUFACTURING ACCREDITATIONS

ISO 9001:2008

ISO 13485:2003

EN ISO 13485:2003

WARNING: Carmustine and Thiotepa, at the tested concentration, degraded Paloma nitrile glove at 15.1 minutes and 15.4 minutes, respectively. The safe use of gloves in chemotherapy treatment is solely the decision of clinicians authorised to make such decision.

MATERIAL SAFETY DATA SHEET



SECTION 1: PRODUCT IDENTIFICATION

| | |
|--|---|
| NAME Hartalega Sdn. Bhd. | ADDRESS C-G-9, Jalan Dataran SD1, Dataran SD, PJU 9, Bandar Sri Damansara, 52200 Kuala Lumpur |
| TELEPHONE NUMBER (603) 6277 1733 | DATE PREPARED October 15, 2014 |
| COMMON NAME (USED ON LABEL) Nitrile Powder Free Examination Gloves | CHEMICAL FAMILY Carboxylated Butadiene Acrylonitrile Polymer Latex |
| APPLICATION Medical and Dental | TRADENAME & SYNONYM GLOVEON COATS NITRILE (CTS38) NITRILE POWDER FREE EXAMINATION GLOVES COATS |

SECTION 2: HAZARDOUS INGREDIENTS

| HAZARDOUS COMPONENT | CAS # | %(WT) | TLV | PEL |
|---------------------|-------|-------|-----|-----|
| N/A | N/A | N/A | N/A | N/A |

PEL: Permissible Exposure Limit established by Occupational Safety and Health Administration (OSHA).
TLV: Threshold Limit Value established by the American Conference of Governmental Industrial Hygienists, 1987-1988.

SECTION 3: COMPOSITION/ INFORMATION ON INGREDIENTS

CHEMICAL COMPOSITION

All chemicals used are non-toxic/ non-hazardous.
Butadiene-Acrylonitrile Latex, Sodium Dodecylbenzenesulfonate, Sulphur, Zinc Oxide, Zinc Di-n-butylthiocarbamate, Titanium Dioxide, Paraffin Wax Emulsion

Coating Ingredient

Colloidal Oatmeal & Constituents, Sodium Benzoate, Processing Aid

SECTION 4: FIRST AID MEASURE

If reaction in the form of skin irritation is noticed, remove gloves immediately and wash affected part with saline water. If there is no relief, seek medical reactions.

SECTION 5: FIRE FIGHTING MEASURE

| FLASHPOINT | AUTOIGNITION TEMPERATURE | FLAMMABLE LIMITS IN AIR |
|------------|--------------------------|-------------------------|
| N/A | N/A | N/A |

EXTINGUISHING MEDIA

Chemical foam and dry chemical may be used.

FIRE-FIGHTING PROCEDURES

Use standard procedures for combustion material fires, including approved self-contained breathing apparatus.

FIRE AND EXPLOSION HAZARDS

No fire or explosion hazards are associated with these products. They will melt at elevated temperatures.

SECTION 6: ACCIDENTAL RELEASE MEASURES

BIOCOMPATABILITY

The chemical formulation of the gloves and surface lubrication materials does not contain any substances normally known to be harmful to the user or to any person with whom the gloves come into contact.

MEDICAL CONDITIONS GENERALLY AGGRAVATED BY EXPOSURE

Nitrile Powder Free Gloves are not expected to cause any adverse health effects.

SECTION 7: HANDLING AND STORAGE

PRECAUTIONS TO BE TAKEN IN HANDLING AND STORAGE

Store in a dry, cool and ventilated area. Do not store above 104 °F (40 °C). Shield open box from direct sunlight, fluorescent lighting and x-rays. Improper storage will decrease usable life.

| SECTION 8: EXPOSURE CONTROLS/ PERSONAL PROTECTION | | | | | |
|---|----------------------------|---|---|-------------------------------------|----------------|
| EYE PROTECTION Not necessary under conditions of intended use. | | | SKIN PROTECTION Not necessary under conditions of intended use. | | |
| RESPIRATORY PROTECTION Not necessary under conditions of intended use. | | | VENTILATION Not necessary under conditions of intended use. | | |
| STEPS TO BE TAKEN IN CASE MATERIAL IS LEAKED OR SPILLED These products are solid articles and are not subject to leaks or spills. | | | | | |
| SECTION 9: PHYSICAL AND CHEMICAL PROPERTIES | | | | | |
| APPEARANCE/ ODOR Ambidextrous, Beaded Cuff, Micro-textured, Chlorinated, Powder Free, Coated with Colloidal Oatmeal USP Skin Protectant, Dawn Blue. | | | | | |
| DIMENSION | X-SMALL | SMALL | MEDIUM | LARGE | X-LARGE |
| Length (mm) | Minimum 230 (same for all) | | | | |
| Width (mm) | 76 ± 4 | 86 ± 4 | 98 ± 4 | 107 ± 4 | 115 ± 4 |
| THICKNESS (mm) - SINGLE WALL MEASUREMENT (same for all) | | | | | |
| Finger (mm) | 0.09 ± 0.02 | | | | |
| Palm (mm) | 0.07 ± 0.02 | | | | |
| TENSILE PROPERTIES | | UNAGED | | AGED | |
| Tensile Strength (Mpa) | | Min. 18.0 MPa | | Min. 16.0 MPa | |
| Ultimate Elongation (%) | | Min. 500% | | Min. 400% | |
| SECTION 10: STABILITY AND REACTIVITY | | | | | |
| BOILING POINT N/A | | VAPOR PRESSURE (mm Hg) N/A | | VAPOR DENSITY (air=1) N/A | |
| SPECIFIC GRAVITY (water=1) N/A | | SOLUBILITY IN WATER Insoluble | | % VOLATILE BY VOLUME N/A | |
| EVAPORATION RATE N/A | | | VISCOSITY N/A | | |
| SECTION 11: TOXICOLOGICAL INFORMATION | | | | | |
| STABILITY Stable. | | | CONDITIONS TO AVOID Does not apply. | | |
| INCOMPATIBILITY (MATERIALS TO AVOID) High polar solvent like methyl ethyl ketone, acetone. | | | | | |
| HAZARDOUS DECOMPOSITION PRODUCTS In a fire, these products may produce a black smoke. Carbon Dioxide, Carbon Monoxide, Oxides of Nitrogen, aromatic/aliphatic hydrocarbons. | | | | | |
| HAZARDOUS POLYMERIZATION Will not occur. | | | | | |
| SECTION 12: ECOLOGICAL INFORMATION | | | | | |
| N/A | | | | | |
| SECTION 13: DISPOSAL CONSIDERATION | | | | | |
| WASTE DISPOSAL METHOD Consult current local, state and federal regulations for proper disposal methods. | | | | | |
| SECTION 14: TRANSPORT INFORMATION | | | | | |
| N/A | | | | | |
| SECTION 15: REGULATORY INFORMATION | | | | | |
| N/A | | | | | |
| SECTION 16: OTHER INFORMATION | | | | | |
| RECOMMENDED USE AND RESTRICTION The Nitrile Powder Free Gloves is a Single Use device. | | | | | |


The Brand

[Leadership](#) | [Certifications](#) | [Global Locations](#)

Certifications

Certifications

Gloveon's quality standards, management systems and exemplary regulatory compliance, all contribute to the global success of the company. Our capabilities have been assessed and certified by the following international governing bodies.

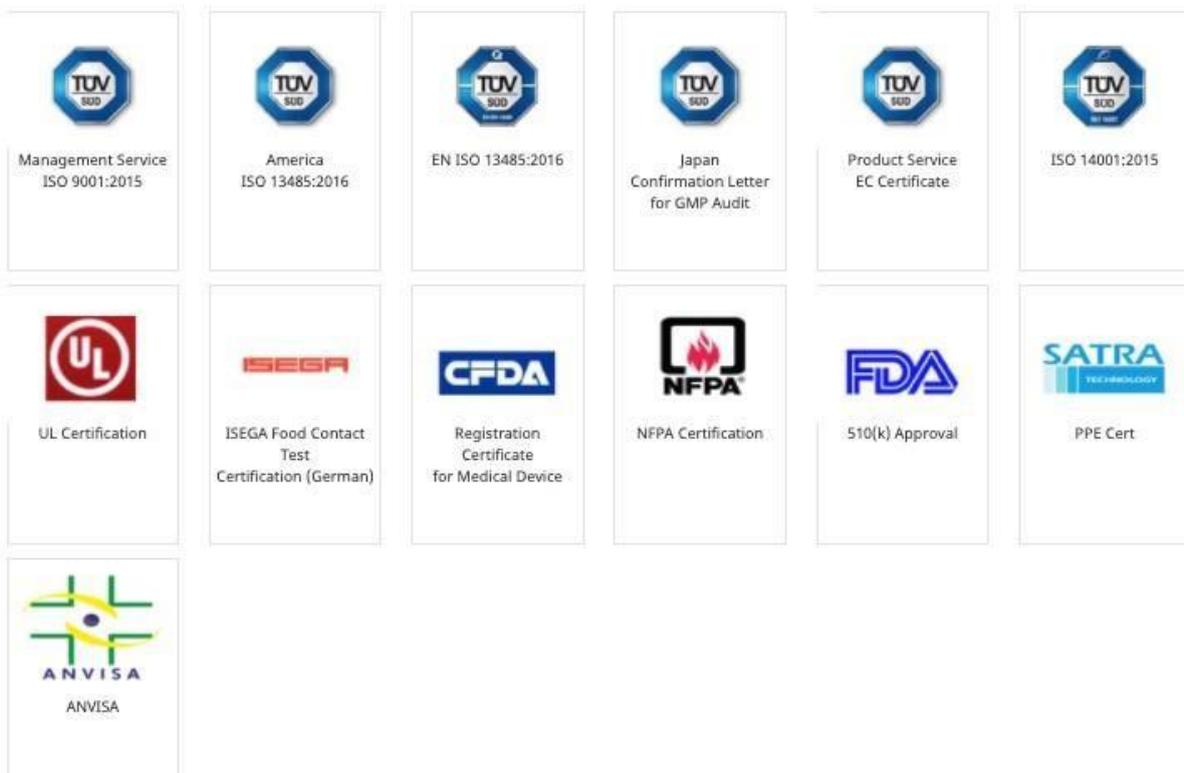



Notified Body: 2777

SATRA customer number P0130

EU Type-Examination Certificate

Certificate number: 2777/10648-04/E04-01

This EU Type-Examination Certificate covers the following product group(s) supported by testing to the relevant standards / technical specifications and examination of the technical file documentation:

Following the EU Type-Examination this product group has been shown to satisfy the applicable essential health and safety requirements of Annex II of the PPE Regulation (EU) 2016/425 as a Category III product.

Product reference: Description

AS NPF Nitrile examination powder free -25.6

Sizes 6 (XS) – 10 (XL) **Classification** **Level** **EN374- 3.1**

37 % Formaldehyde 6 %

40 % Sodium 6 %

30 % Hydrogen 2 %

EN ISO 374-1:2016/Type 17.0

EN ISO 374-

Resistance to Bacteria and Fungi Pass

Resistance to Virus Pass

Standards/Technical specifications applied

EN 420: 2003+A1: 2009; EN ISO 374-1:2016; EN ISO 374-5:2016

Technical reports/Approval documents:

SATRA: CHM0265112/1749/EN/A, CHM0265112/1749/EN/B, CHM0265112/1749/SPT, CHM0272621/1826/JS, CHM0275215/1836/LH, CHM0275215/1836/LH/E, CHM0275215/1836/LH/D, CHM0275215/1836/LH/A/Final
TUV: 7191143339-CHM16-01-RC

Signed on behalf of SATRA:

Date of issue: 17/04/2019

Expiry date: 25/06/2023

SATRA Technology Europe Limited. Bracetown Business Park. Clonee. D15YN2P. Republic of Ireland.

EC Declaration of Conformity

We, the manufacturer

Hartalega Sdn. Bhd.,
No. 7, Kawasan Perusahaan Suria,
45600 Bestari Jaya,
Selangor Darul Ehsan,
Malaysia

with European Representative

Medical Device Safety Service (MDSS)
Schiffgraben 41, 30175 Hannover,
Germany

Declares that the new PPE described hereafter

Category III (Type B)
HSB-TF-009
Nitrile Powder Free Gloves with Colloidal Oatmeal USP Skin Protectant

is in conformity with the relevant Union harmonisation legislation

PPE Regulation (EU) 2016/425

where such is the case, with the national standard transposing harmonized standard number

EN 420: 2003+A1: 2009
EN ISO 374 - 1:2016
EN ISO 374 - 5:2016

The notified body SATRA Technology Centre with Notified Body Number of 2777 performed the EU type-examination (Module B) and issued the EU type-examination certificate 2777/10783-02/E00-00.

The PPE is subject to the conformity assessment procedure conformity to type based on internal production control plus supervised product checks at random intervals (Module C2) under surveillance of the Notified body SATRA Technology Centre with Notified Body Number of 2777.

Done at Hartalega Sdn. Bhd. on 11th February 2020.



Kuan Eu Jin
Quality Management Representative



Hartalega Sdn Bhd
Nurul Kong
Quality Assurance Senior Manager
No. 7, Kawasan Perusahaan Suria
Bestari Jaya, 45600 My

Re: K180644

Trade/Device Name: Nitrile Powder Free Examination Gloves with Colloidal Oatmeal -Lemon Green
Regulation Number: 21 CFR 880.6250
Regulation Name: Patient Examination Glove
Regulatory Class: Class I
Product Code: LZA
Dated: July 16, 2018
Received: July 23, 2018

Dear Nurul Kong:

We have reviewed your Section 510(k) premarket notification of intent to market the device referenced above and have determined the device is substantially equivalent (for the indications for use stated in the enclosure) to legally marketed predicate devices marketed in interstate commerce prior to May 28, 1976, the enactment date of the Medical Device Amendments, or to devices that have been reclassified in accordance with the provisions of the Federal Food, Drug, and Cosmetic Act (Act) that do not require approval of a premarket approval application (PMA). You may, therefore, market the device, subject to the general controls provisions of the Act. Although this letter refers to your product as a device, please be aware that some cleared products may instead be combination products. The 510(k) Premarket Notification Database located at <https://www.accessdata.fda.gov/scripts/cdrh/cfdocs/cfpmn/pmn.cfm> identifies combination product submissions. The general controls provisions of the Act include requirements for annual registration, listing of devices, good manufacturing practice, labeling, and prohibitions against misbranding and adulteration. Please note: CDRH does not evaluate information related to contract liability warranties. We remind you, however, that device labeling must be truthful and not misleading.

If your device is classified (see above) into either class II (Special Controls) or class III (PMA), it may be subject to additional controls. Existing major regulations affecting your device can be found in the Code of Federal Regulations, Title 21, Parts 800 to 898. In addition, FDA may publish further announcements concerning your device in the [Federal Register](#).

Please be advised that FDA's issuance of a substantial equivalence determination does not mean that FDA has made a determination that your device complies with other requirements of the Act or any Federal statutes and regulations administered by other Federal agencies. You must comply with all the Act's requirements, including, but not limited to: registration and listing (21 CFR Part 807); labeling (21 CFR Part 801); medical device reporting (reporting of medical device-related adverse events) (21 CFR 803) for

U.S. Food & Drug Administration
12005 New Hampshire Avenue
Silver Spring, MD 20993 www.fda.gov

Page 2 - Nurul Kong

K180644

devices or postmarketing safety reporting (21 CFR 4, Subpart B) for combination products (see <https://www.fda.gov/CombinationProducts/GuidanceRegulatoryInformation/ucm597488.htm>); good manufacturing practice requirements as set forth in the quality systems (QS) regulation (21 CFR Part 820) for devices or current good manufacturing practices (21 CFR 4, Subpart A) for combination products; and, if applicable, the electronic product radiation control provisions (Sections 531-542 of the Act); 21 CFR 1000-1050.

Also, please note the regulation entitled, "Misbranding by reference to premarket notification" (21 CFR Part 807.97). For questions regarding the reporting of adverse events under the MDR regulation (21 CFR Part 803), please go to <http://www.fda.gov/MedicalDevices/Safety/ReportaProblem/default.htm>.

For comprehensive regulatory information about medical devices and radiation-emitting products, including information about labeling regulations, please see Device Advice (<https://www.fda.gov/MedicalDevices/DeviceRegulationandGuidance/>) and CDRH Learn (<http://www.fda.gov/Training/CDRHLearn>). Additionally, you may contact the Division of Industry and Consumer Education (DICE) to ask a question about a specific regulatory topic. See the DICE website (<http://www.fda.gov/DICE>) for more information or contact DICE by email (DICE@fda.hhs.gov) or phone (1-800-638-2041 or 301-796-7100).

Sincerely,

Clarence W. Murray III -S

For Tina Kiang, Ph.D.
Acting Director
Division of Anesthesiology,
General Hospital, Respiratory,
Infection Control, and Dental Devices
Office of Device Evaluation
Center for Devices and Radiological Health

Enclosure

| | |
|---|---|
| DEPARTMENT OF HEALTH AND HUMAN SERVICES Food and Drug Administration Indications for Use | Form Approved: OMB No. 0910-0120 Expiration Date: 06/30/2020 See PRA Statement below. |
| 510(k) Number (if known) K180644 | |
| Device Name Nitrile Powder Free Examination Glove with Colloidal Oatmeal - Lemon Green | |
| Indications for Use (Describe) The Nitrile Powder Free Examination Glove with Colloidal Oatmeal - Lemon Green is a non-sterile disposable device intended for medical purpose that is worn on the examiner's hand to prevent contamination between patient and examiner. | |
| <hr/> Type of Use (Select one or both, as applicable) <input type="checkbox"/> Prescription Use (Part 21 CFR 801 Subpart D) <input checked="" type="checkbox"/> Over-The-Counter Use (21 CFR 801 Subpart C) | |
| CONTINUE ON A SEPARATE PAGE IF NEEDED. | |
| This section applies only to requirements of the Paperwork Reduction Act of 1995. "DO NOT SEND YOUR COMPLETED FORM TO THE PRA STAFF EMAIL ADDRESS BELOW." The burden time for this collection of information is estimated to average 79 hours per response, including the time to review instructions, search existing data sources, gather and maintain the data needed and complete and review the collection of information. Send comments regarding this burden estimate or any other aspect of this information collection, including suggestions for reducing this burden, to: Department of Health and Human Services Food and Drug Administration Office of Chief Information Officer Paperwork Reduction Act (PRA) Staff PRAStaff@fda.hhs.gov <i>"An agency may not conduct or sponsor, and a person is not required to respond to, a collection of information unless it displays a currently valid OMB number."</i> | |
| FORM FDA 3881 (7/17) | Page 1 of 1 |



510(k) Premarket Notification

[FDA Home](#)
[Medical Devices](#)
[Databases](#)



[510\(k\)](#) | [DeNovo](#) | [Registration & Listing](#) | [Adverse Events](#) | [Recalls](#) | [PMA](#) | [HDE](#) | [Classification](#) | [Standards](#)
[CFR Title 21](#) | [Radiation-Emitting Products](#) | [X-Ray Assembler](#) | [Medsun Reports](#) | [CLIA](#) | [TPLC](#)

[New Search](#)
[Back To Search Results](#)

Device Classification Name [Polymer Patient Examination Glove](#)
510(K) Number K133956
Device Name NITRILE POWDER FREE EXAMINATION GLOVE WITH COLLOIDAL OATMEAL USP SKIN PROTECTANT DRUG - WHITE / DAWN BLUE / LEMON GREEN
Applicant HARTALEGA SDN BHD
 NO. 7, KAWASAN PERUSAHAAN SURIA
 Bestari Jaya, Selangor, MY 45600
Applicant Contact Nurul Aisyah Kong
Correspondent HARTALEGA SDN BHD
 NO. 7, KAWASAN PERUSAHAAN SURIA
 Bestari Jaya, Selangor, MY 45600
Correspondent Contact Nurul Aisyah Kong
Regulation Number [880.6250](#)
Classification Product Code [LZA](#)
Date Received 12/23/2013
Decision Date 05/28/2014
Decision Substantially Equivalent (SESE)
Regulation Medical Specialty General Hospital
510k Review Panel General Hospital
Summary [Summary](#)
Type Traditional
Reviewed By Third Party No
Combination Product No

| FDA Home ³ Medical Devices⁴ Databases⁵ 510(K) Premarket Notification 1 to 16 of 92 Results for Hartalega | | | |
|---|-------------------------------------|---|---|
| 1 2 ⁶ 3 ⁷ 4 ⁸ 5 ⁹ 6 ¹⁰ 7 ¹¹ 8 ¹² 9 ¹³ >14 | | | |
| 10 results per page | | | |
| New Search ¹⁵ Export To Excel Help¹⁶ | | | |
| Device Name <small>▲17 ▼18</small> | Applicant <small>▲19 ▼20</small> | 510(K) Number <small>▲21 ▼22</small> | Decision Date <small>▲23 ▼24</small> |
| Powdered Sterile Latex Surgical Glove, With Protein Content Labeling Claim (200 Micrograms Or Less) | HARTALEGA SDN BHD | K001959 | 07/26/2000 |
| Powder Free Sterile Latex Surgical Gloves, Contains 50 Microgram Or Less Of Total Water Extractable Protein Per Gram | HARTALEGA SDN BHD | K002593 | 11/29/2000 |
| Freeform Blue Powderfree Nitrile Examination Gloves | HARTALEGA SDN BHD | K022671 | 11/18/2002 |
| Freeform Blue Powder-free Nitrile Examination Gloves | HARTALEGA SDN BHD | K041391 | 07/09/2004 |
| Nitrile Powder Free Examination Gloves (White) | HARTALEGA SDN BHD | K050214 | 03/16/2005 |
| Nitrile Powdered Examination Gloves (White) | HARTALEGA SDN BHD | K050215 | 03/11/2005 |
| Chlorinated Powder Free Latex Examination Gloves (Yellow) | HARTALEGA SDN BHD | K050277 | 06/07/2005 |
| Nitrile Powder Free Examination Gloves (Blue) | HARTALEGA SDN BHD | K051777 | 08/12/2005 |

1 of 4 5/15/2020, 5:04 PM

Testing. Development. Problem Solving.



April 15, 2009

• TEST REPORT •

PN 83672A - Amended

CHEMICAL ANALYTICAL SERVICES

Prepared For:
Hartalega SDN. BDH
Ms. Nurul Aisyah Kong
No. 7 Kawasan Perusahaan Suria
Bestari Jaya
Selangor, 45600
Malaysia

Prepared By: 
Tiffany L. Heller
Chemical Technician

Approved By: 
Ana C. Barbur, M.S.
Manager, Chemical & Pharmaceutical Services



An AZLA Accredited Testing Laboratory — Certificate Numbers 255.01 & 255.02
ISO 9001:2000 Registered
Member of ACIL, The American Council of Independent Laboratories

ISO 9001:2000
Registered



Letters and reports are for the exclusive use of the clients to whom they are submitted and shall not be reproduced, stored in a retrieval system, or used in any way without the written permission of Akron Rubber Development Laboratory, Inc. (ARDL). The information contained herein applies to the specific material, product or processes tested or evaluated. No warranty of any kind is herein (expressed or implied). The liability of ARDL, Inc. shall be limited to the amount of compensation paid for services. ARDL, Inc. is accredited by AZLA for the test methods listed on the attached scope.

www.ardl.com

2887 Gilchrist Rd. | Akron, Ohio 44305 | answers@ardl.com
Toll Free (800) 830-ARDL | Worldwide (330) 794-6600 | Fax (330) 794-6610



Testing, Development, Problem Solving.

April 15, 2009

Ms. Nurul Aisyah Kong
Hartalega SDN. BHD

Page 1 of 3 - PN 83672A - Amended

SUBJECT: Permeation testing per ASTM D 6978-05 on sample submitted by the above company. Wire Transfer.

RECEIVED: Glove sample identified as Nitrile Powder Free Examination Gloves (Blue) Code: ABLU.

TESTING CHEMOTHERAPY DRUGS:

Table 1. List of the Testing Chemotherapy Drugs, Sources, and Expiration Dates

| TESTING CHEMOTHERAPY DRUGS | DRUG SOURCE |
|----------------------------|--|
| Carmustine (BCNU) | Sigma, Lot# 038K4008, Expiration 12/2009 |
| Cisplatin | Sigma, Lot# 59H3657, Expiration 09/2009 |
| Cyclophosphamide (Cytoxan) | Sigma, Lot# 068K1131, Expiration 1/2010 |
| Dacarbazine (DTIC) | Hospira, Lot# U022233AA, Expiration 06/2010 |
| Doxorubicin Hydrochloride | Teva, Lot# 7N625, Expiration 10/2009 |
| Etoposide (Teposar) | Teva, Lot# 313039768, Expiration 9/2011 |
| Fluorouracil | APP, Lot# 203867, Expiration 03/2010 |
| Mitomycin C | Sigma, Lot# 048K1086, Expiration 01/2010 |
| Methotrexate | Hospira, Lot# U024457AA, Expiration 05/2010 |
| Paclitaxel (Taxol) | Dabur Oncology, Lot# PAJ08H00701, Exp. 05/2010 |
| Thiotepa | Sigma, Lot# 078K1526, Expiration 12/2009 |
| Vincristine Sulfate | Hospira, Lot# U037139AA, Expiration 12/2009 |

COLLECTION MEDIA:

The collection media, which were selected, are listed in Table 2.

Table 2. Collection Media for Testing Chemotherapy Drugs

| TEST DRUG AND CONCENTRATION | COLLECTION MEDIUM |
|---|-----------------------------------|
| Carmustine (BCNU), 3.3 mg/ml (3,300 ppm) | 10% Ethanol Aqueous Solution |
| Cisplatin, 1.0 mg/ml (1,000 ppm) | Distilled Water |
| Cyclophosphamide (Cytoxan), 20 mg/ml (20,000 ppm) | Distilled Water |
| Dacarbazine (DTIC), 10.0 mg/ml (10,000 ppm) | Distilled Water |
| Doxorubicin Hydrochloride, 2.0 mg/ml (2,000 ppm) | Distilled Water |
| Etoposide (Teposar), 20.0 mg/ml (20,000 ppm) | Distilled Water |
| Fluorouracil, 50.0 mg/ml (50,000 ppm) | 9.20 pH Sodium Hydroxide Solution |
| Methotrexate, 25 mg/ml (25,000 ppm) | Distilled Water |
| Mitomycin C, 0.5 mg/ml (500 ppm) | Distilled Water |
| Paclitaxel (Taxol), 6.0 mg/ml (6,000 ppm) | 30% Methanol Aqueous Solution |
| Thiotepa, 10.0 mg/ml (10,000 ppm) | Distilled Water |
| Vincristine Sulfate, 1.0 mg/ml (1,000 ppm) | Distilled Water |

www.ardl.com

2887 Glacrist Rd. | Akron, Ohio 44305 | answers@ardl.com
Toll Free (800) 830-ARDL | Worldwide (330) 794-6600 | Fax (330) 794-6610



MDSS - Schiffgroben 41 - 30175 Hannover, Germany

Hartalega NGC Sdn. Bhd.
Khairunnisa Wvarsito
No. 1, Persiaran Tanjung
Kawasan Perindustrian Tanjung
43900 Sepang, Selangor
MALAYSIA

Schiffgroben 41
30175 Hannover, Germany
Tel: + 49 - 511 - 62 62 86 30
Fax: + 49 - 511 - 62 62 86 33
eMail: info@mdss.com
Internet: www.mdss.com

2019.01.18

Confirmation of CE Registration

Dear Khairunnisa,

It is our pleasure to enclose the new Certificate of CE-Registration for your product.

Please note that registration was performed under § 25 MPG (Medizinproduktegesetz). This is the *Federal Republic of Germany's national interpretation of Medical Device Directive 93/42/EEC*. Registration is therefore in accordance with EU legislation. We remind you that all products must meet the applicable provision of the European and national regulation before they may be placed on the market.

We are looking forward to continuing our good business relationship and wish you a successful product launch in Europe.

Best regards,

Juan Monferrer Tena
Administrative Assistant
Medical Device Safety Service GmbH

Encl.
1 Certificate of CE-Registration
1 Annex A

MDSS - Medical Device Safety Service GmbH
Handelsregister: Hannover HRB 57318 - US-IdNr. DE 177346163 - Geschäftsführer: Ludger Möller
Bankverbindungen
Sparkasse Hannover
S.W.I.F.T.: SPKHDE33
IBAN: DE24 2505 0180 0910 0792 77
Commerzbank AG, Hannover
S.W.I.F.T.: COBDE333
IBAN: DE07 2504 0050 0338 8810 00



Certificate of CE-Registration



This is to certify that, in accordance with the Medical Device Directive 93/42/EEC, Medical Device Safety Service GmbH (MDSS) agrees to perform all duties and responsibilities as the Authorized Representative for:

Hartalega NGC Sdn. Bhd.
No. 1, Persiaran Tanjung
Kawasan Perindustrian Tanjung
43900 Sepang, Selangor
MALAYSIA

as stipulated and demanded by the aforementioned Directive. The German Competent Authority has allocated the medical devices of the Manufacturer registration numbers as foreseen in:

Annex A dated January 18, 2019

The Manufacturer has provided MDSS with the appropriate Declaration(s) of Conformity confirming that the medical devices fulfill the applicable requirements of Directive 93/42/EEC. In compliance with German law, a safety officer has been appointed for Germany.

2019-01-18

Ludger Möller
President
MDSS GmbH



April 25, 2020

Hartalega NGC SDN. BHD.
Nurul Kong
Senior Manager- Quality Assurance
Kawasan Perindustrian Tanjung
Sepang, Selangor 43900
Malaysia

Re: K200581

Trade/Device Name: Biodegradable Nitrile Powder Free Examination Gloves Tested for Use with Chemotherapy Drugs and Fentanyl Citrate (Blue)
Regulation Number: 21 CFR 880.6250
Regulation Name: Non-Powdered Patient Examination Glove
Regulatory Class: Class I, reserved
Product Code: LZA, LZC, QDO
Dated: February 27, 2020
Received: March 5, 2020

Dear Nurul Kong:

We have reviewed your Section 510(k) premarket notification of intent to market the device referenced above and have determined the device is substantially equivalent (for the indications for use stated in the enclosure) to legally marketed predicate devices marketed in interstate commerce prior to May 28, 1976, the enactment date of the Medical Device Amendments, or to devices that have been reclassified in accordance with the provisions of the Federal Food, Drug, and Cosmetic Act (Act) that do not require approval of a premarket approval application (PMA). You may, therefore, market the device, subject to the general controls provisions of the Act. Although this letter refers to your product as a device, please be aware that some cleared products may instead be combination products. The 510(k) Premarket Notification Database located at <https://www.accessdata.fda.gov/scripts/cdrh/cfdocs/cfpmm/pmm.cfm> identifies combination product submissions. The general controls provisions of the Act include requirements for annual registration, listing of devices, good manufacturing practice, labeling, and prohibitions against misbranding and adulteration. Please note: CDRH does not evaluate information related to contract liability warranties. We remind you, however, that device labeling must be truthful and not misleading.

If your device is classified (see above) into either class II (Special Controls) or class III (PMA), it may be subject to additional controls. Existing major regulations affecting your device can be found in the Code of Federal Regulations, Title 21, Parts 800 to 898. In addition, FDA may publish further announcements concerning your device in the [Federal Register](#).

Please be advised that FDA's issuance of a substantial equivalence determination does not mean that FDA has made a determination that your device complies with other requirements of the Act or any Federal

U.S. Food & Drug Administration
10801 New Hampshire Avenue
Silver Spring, MD 20993
<https://www.fda.gov>

2K200581 - Nurul Kong

Page

statutes and regulations administered by other Federal agencies. You must comply with all the Act's requirements, including, but not limited to: registration and listing (21 CFR Part 807); labeling (21 CFR Part 801); medical device reporting (reporting of medical device-related adverse events) (21 CFR 803) for devices or postmarketing safety reporting (21 CFR 4, Subpart B) for combination products (see <https://www.fda.gov/combo-products/mda/ndc-regulatory-information-postmarketing-safety-reporting-combination-products>); good manufacturing practice requirements as set forth in the quality systems (QS) regulation (21 CFR Part 820) for devices or current good manufacturing practices (21 CFR 4, Subpart A) for combination products; and, if applicable, the electronic product radiation control provisions (Sections 531-542 of the Act); 21 CFR 1000-1050.

Also, please note the regulation entitled, "Misbranding by reference to premarket notification" (21 CFR Part 807.97). For questions regarding the reporting of adverse events under the MDR regulation (21 CFR Part 803), please go to <https://www.fda.gov/medical-devices/medical-device-safety/medical-device-reporting-ndc-how-report-medical-device-problems>.

For comprehensive regulatory information about medical devices and radiation-emitting products, including information about labeling regulations, please see Device Advice (<https://www.fda.gov/medical-devices/device-advice-comprehensive-regulatory-assistance>) and CDRLearn (<https://www.fda.gov/training-and-continuing-education/cdrh-learn>). Additionally, you may contact the Division of Industry and Consumer Education (DICE) to ask a question about a specific regulatory topic. See the DICE website (<https://www.fda.gov/medical-devices/device-advice-comprehensive-regulatory-assistance/contact-us/division-industry-and-consumer-education-dice>) for more information or contact DICE by email (DICE@fda.hhs.gov) or phone (1-800-638-2041 or 301-796-7100).

Sincerely,

Elizabeth F. Claverie

CAPT Elizabeth Claverie, M.S.

Assistant Director

DHT4B: Division of Infection Control

and Plastic Surgery Devices

OHT4: Office of Surgical

and Infection Control Devices

Office of Product Evaluation and Quality

Center for Devices and Radiological Health

Enclosure



Hartalega Attains International Certification on Occupational Health and Safety – OHSAS 18001



Hartalega has once again proven its commitment to the highest quality standards, as the Group recently attained OHSAS 18001:2007 certification.

Awarded by TUV SUD Asia Pacific TUV SUD Group, an audit and management systems certification body, OHSAS 18001:2007 is an internationally recognised standard which sets the requirements and best practices for occupational health and safety management systems in an organisation. The Group was previously awarded ISO 14001:2004 certification as a result of its outstanding environmental management system.

Mr Kuan Mun Leong, Managing Director of Hartalega said, "The OHSAS is a testament to our group's commitment to the well being of all Hartanians. As we continue to grow our business aggressively, being able to provide a quality work place in the aspects of health and safety is very important."

The OHSAS 18001:2007 certification was achieved through Hartalega's comprehensive range of health and safety measures, which include internal workplace audits, risk assessments, behaviour observations, accident and incident investigations, work permit issuances, training sessions for emergency preparedness and environmental performance monitoring, amongst others.

"As important as it is to focus on productivity and efficiency, it is equally as crucial to ensure that our employees work in a safe environment. We aim to continuously enhance Health, Safety and Environment initiatives throughout the Group for the benefit of our workforce," concluded Kuan.



CRS REF : SAT/18/0248
 DATE RECEIVED : MAR 02, 2018
 DATE REPORTED: MAR 14, 2018
 PAGE: 1 of 1

Report No. : CRSSA/02645/18

TEST REPORT

Product Description : Powder Free Nitrile Examination Gloves
 Country of Origin : Malaysia
 Size : Medium
 Quantity Tested : 200 pieces
 Test Conducted : Freedom from holes
 Test Method : EN455 Part 1:2000
 Testing Period : 02 Mar 2018 - 08 Mar 2018

Based on submitted samples, the following results obtained :-

Acceptable Quality Limit (AQL) : 1.5 Accept : 7 Found : 2

Result : Within AQL

Note: Upon Customer's request, this report has been issued in more than one original. Only the first original is a legally binding document and may be used for any legal purpose, including payment. (Original 1-3)

SGS (MALAYSIA) SDN. BHD.

CHEE TUCK CHOON
 B.Sc. MMIC
 SECTION HEAD

This document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/Forms-and-Conditions.aspx> and, for signature formal documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/Forms-and-Conditions.aspx#ElectronicDocuments>. Attention is drawn to the limitations of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that administrative control remains with the Company's findings at the time of its issuance only and within the limits of Client's instructions, if any. The Company's sole responsibility is to the Client and this document does not constitute advice or a statement of fact, nor does it constitute an offer of insurance or any other financial product. This document cannot be reproduced, copied or used, without prior written approval of the Company. Any unauthorised alteration, forgery or falsification of the content or appearance of this document is severely prohibited and may be prosecuted to the fullest extent of the law. Clients elsewhere shall be made aware in the last report (and only in the last report) of the location and date stamping of the original report samples of three months only.

SGS (Malaysia) Sdn. Bhd. Lot 4, Persiaran Jabi Perak, Seksyen 22, 42000 Shah Alam, Selangor, Malaysia
 (Company No. 10871-1) t +6 (03) 5481 8282 f +6 (03) 5481 8215 www.sgs.com

Member of the SGS Group (SGS SA)



CRS REF : SAT/18/0248
 DATE RECEIVED : MAR 02, 2018
 DATE REPORTED: MAR 14, 2018
 PAGE: 1 of 1

Report No. : CRSSA/02646/18

TEST REPORT

Product Description : Powder Free Nitrile Examination Gloves
 Country of Origin : Malaysia
 Size : Medium
 Quantity Tested : 13 pieces
 Test Conducted : Dimensions
 Test Method : EN 455 Part 2:2015
 Testing Period : 02 Mar 2018 - 08 Mar 2018

Based on submitted samples, the following results obtained :-

| Size | M | M | M | M | M | M | M | M | M | M | M | M | M | Median |
|--------|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|--------|
| Width | 98 | 98 | 96 | 98 | 98 | 97 | 98 | 97 | 98 | 97 | 96 | 97 | 97 | 97 |
| Length | 250 | 255 | 250 | 255 | 251 | 250 | 252 | 252 | 250 | 254 | 252 | 253 | 252 | 252 |

Note: Upon Customer's request, this report has been issued in more than one original. Only the first original is a legally binding document and may be used for any legal purpose, including payment. (Original 1-3)

SGS (MALAYSIA) SDN. BHD.

CHEE TUCK CHOON
 B.Sc. MMIC
 SECTION HEAD

This document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/Forms-and-Conditions.aspx> and, for signature formal documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/Forms-and-Conditions.aspx#ElectronicDocuments>. Attention is drawn to the limitations of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that administrative control remains with the Company's findings at the time of its issuance only and within the limits of Client's instructions, if any. The Company's sole responsibility is to the Client and this document does not constitute advice or a statement of fact, nor does it constitute an offer of insurance or any other financial product. This document cannot be reproduced, copied or used, without prior written approval of the Company. Any unauthorised alteration, forgery or falsification of the content or appearance of this document is severely prohibited and may be prosecuted to the fullest extent of the law. Clients elsewhere shall be made aware in the last report (and only in the last report) of the location and date stamping of the original report samples of three months only.

SGS (Malaysia) Sdn. Bhd. Lot 4, Persiaran Jabi Perak, Seksyen 22, 42000 Shah Alam, Selangor, Malaysia
 (Company No. 10871-1) t +6 (03) 5481 8282 f +6 (03) 5481 8215 www.sgs.com

Member of the SGS Group (SGS SA)



CRS REF : SAT/18/0248
 DATE RECEIVED : MAR 02, 2018
 DATE REPORTED: MAR 14, 2018
 PAGE: 1 of 1

Report No. : CRSSA/02647/18

TEST REPORT

Product Description : Powder Free Nitrile Examination Gloves
 Country of Origin : Malaysia
 Size : Medium
 Quantity Tested : 13 pieces
 Test Conducted : Force at Break During Shelf Life and After
 Test Method : Challenge EN 455 Part 2:2015
 Agents : 10 ± 2 Deg C for 168 hrs
 Testing Period : 02 Mar 2018 - 14 Mar 2018

| SIZE | SAMPLE NO. | Force at Break, N | |
|--------------------|------------|-------------------|-------------|
| | | BEFORE AGING | AFTER AGING |
| M | 1 | 8.2 | 8.4 |
| | 2 | 8.1 | 8.2 |
| | 3 | 7.9 | 6.5 |
| | 4 | 7.3 | 7.9 |
| | 5 | 8.5 | 6.6 |
| | 6 | 9.2 | 9.3 |
| | 7 | 8.7 | 7.2 |
| | 8 | 8.8 | 7.4 |
| | 9 | 9.3 | 7.1 |
| | 10 | 8.0 | 7.9 |
| | 11 | 9.2 | 7.3 |
| | 12 | 6.3 | 7.1 |
| | 13 | 8.1 | 7.1 |
| Median Requirement | | 8.2 | 7.3 |
| | | 24.0 | 24.0 |

Note: Upon Customer's request, this report has been issued in more than one original. Only the first original is a legally binding document and may be used for any legal purpose, including payment. (Original 1-3)

SGS (MALAYSIA) SDN. BHD.

CHEE TUCK CHOON
 B.Sc. MMIC
 SECTION HEAD

This document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/Forms-and-Conditions.aspx> and, for signature formal documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/Forms-and-Conditions.aspx#ElectronicDocuments>. Attention is drawn to the limitations of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that administrative control remains with the Company's findings at the time of its issuance only and within the limits of Client's instructions, if any. The Company's sole responsibility is to the Client and this document does not constitute advice or a statement of fact, nor does it constitute an offer of insurance or any other financial product. This document cannot be reproduced, copied or used, without prior written approval of the Company. Any unauthorised alteration, forgery or falsification of the content or appearance of this document is severely prohibited and may be prosecuted to the fullest extent of the law. Clients elsewhere shall be made aware in the last report (and only in the last report) of the location and date stamping of the original report samples of three months only.

SGS (Malaysia) Sdn. Bhd. Lot 4, Persiaran Jabi Perak, Seksyen 22, 42000 Shah Alam, Selangor, Malaysia
 (Company No. 10871-1) t +6 (03) 5481 8282 f +6 (03) 5481 8215 www.sgs.com

Member of the SGS Group (SGS SA)



CRS REF : SAT/18/0248
 DATE RECEIVED : MAR 02, 2018
 DATE REPORTED: MAR 14, 2018
 PAGE: 1 of 1

Report No. : CRSSA/02648/18

TEST REPORT

Product Description : Powder Free Nitrile Examination Gloves
 Country of Origin : Malaysia
 Size : Medium
 Quantity Tested : 5 pieces
 Test Conducted : Powder Content
 Test Method : EN455 Part 3:2015
 Testing Period : 02 Mar 2018 - 08 Mar 2018

On testing the samples, the following results were obtained:-

| SIZE | Average Powder Mass per Glove |
|------|-------------------------------|
| M | 0.26 mg |

Note: Upon Customer's request, this report has been issued in more than one original. Only the first original is a legally binding document and may be used for any legal purpose, including payment. (Original 1-3)

SGS (MALAYSIA) SDN. BHD.

CHEE TUCK CHOON
 B.Sc. MMIC
 SECTION HEAD

This document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/Forms-and-Conditions.aspx> and, for signature formal documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/Forms-and-Conditions.aspx#ElectronicDocuments>. Attention is drawn to the limitations of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that administrative control remains with the Company's findings at the time of its issuance only and within the limits of Client's instructions, if any. The Company's sole responsibility is to the Client and this document does not constitute advice or a statement of fact, nor does it constitute an offer of insurance or any other financial product. This document cannot be reproduced, copied or used, without prior written approval of the Company. Any unauthorised alteration, forgery or falsification of the content or appearance of this document is severely prohibited and may be prosecuted to the fullest extent of the law. Clients elsewhere shall be made aware in the last report (and only in the last report) of the location and date stamping of the original report samples of three months only.

SGS (Malaysia) Sdn. Bhd. Lot 4, Persiaran Jabi Perak, Seksyen 22, 42000 Shah Alam, Selangor, Malaysia
 (Company No. 10871-1) t +6 (03) 5481 8282 f +6 (03) 5481 8215 www.sgs.com

Member of the SGS Group (SGS SA)